



Simec AG

Areal Bleiche West Postfach 413 CH - 4800 Zofingen
Telefon +41 62 752 83 08 Fax +41 62 752 83 09
E-Mail: info@simec.ch www.simec.ch

Test report

Number **C 34814**

Object of analysis: **Testosterone decanoate**

Customer:



Samples: 1

Batch:

-

Receipt: 05.08.2015

Subject: **Assay, Identification**

Method(s): **HPLC**

Sample / Analysis:	Method	Status	Result	Specification	complies
<u>Testosterone decanoate:</u>					
Identification	HPLC	N	complies	complies	yes
Content	HPLC	N	98.9 %	≥ 98.5 %	yes

Method-status: G = GMP A = accredited V = generally validated P = validated on product N = not validated
E = external lab

Remarks:

Signatures:

controlled & released:

Staff:

completed:

27.08.2015


page 1 of 1

The enclosed results refer exclusively to the object of examination described above.
The measuring accuracy is available on request. Only handwritten signatures are valid.
Without written permission, it is not allowed to publish single parts of this report.

Report steroid analysis

HPLC: Nr.5
 Analysendatum: 24.08.2015 09:56:40
 Vial: 39
 Probenidentifikation: C34814 A
 Operator: admin
 Chrom.-Beding. ACN / Wasser, gradient
 Temperatur: 40 °C
 Säule Nr. 88, 250 x 4,6, C18
 Detektion: UV 240nm

Druckdatum: 24.08.2015 17:24:30
 Injektvolumen: 20

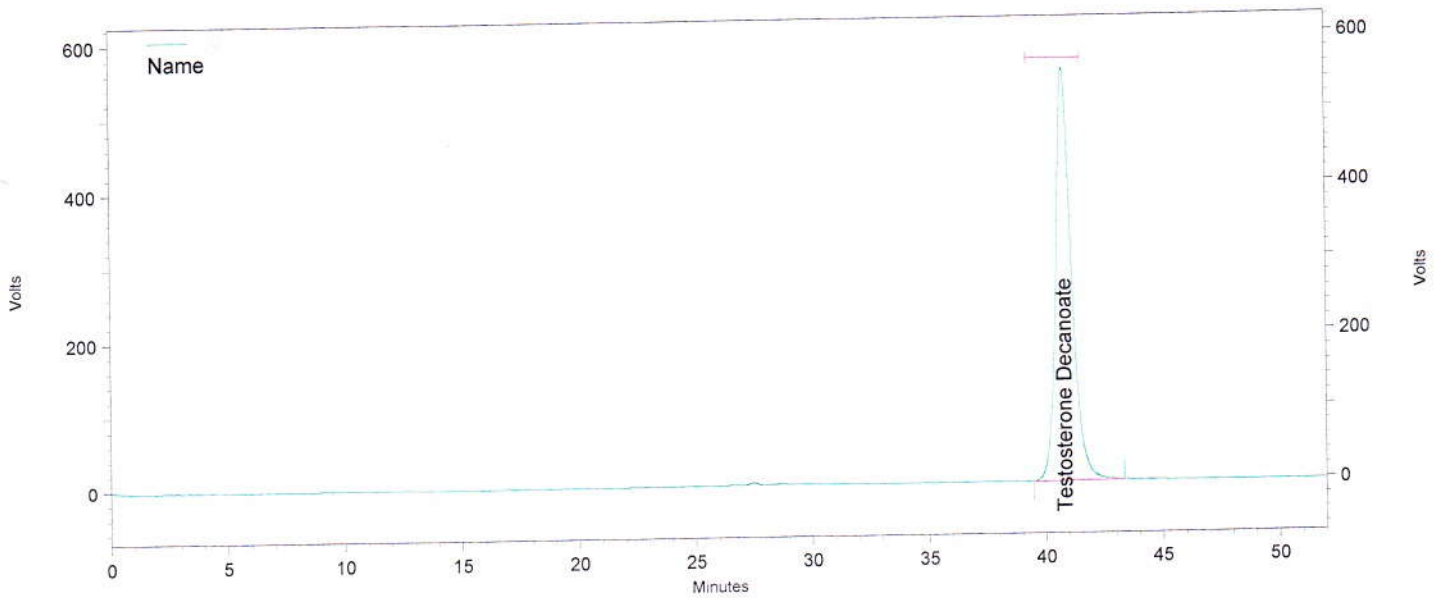

Channel A

UV Results


Name	Time	Area	Amount	Area Percent
Testosterone propionate			0,000 BDL	
Testosterone Phenylpropionate			0,000 BDL	
Testosterone isocaproate			0,000 BDL	
Testosterone Decanoate	40,770	103199292	0,000	100,000
Totals		103199292	0,000	100,000

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2015\August 2015\Diverse Steroide\18,08,15\24.08.2015 09-55-25_C34814 A-Rep1.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC: Nr.5
 Analysendatum: 24.08.2015 10:50:10
 Vial: 39
 Probenidentifikation: C34814 A
 Operator: admin
 Chrom.-Beding. ACN / Wasser, gradient
 Temperatur: 40 °C
 Säule Nr. 88, 250 x 4,6, C18
 Detektion: UV 240nm

Druckdatum: 24.08.2015 17:24:41
 Injektvolumen: 20

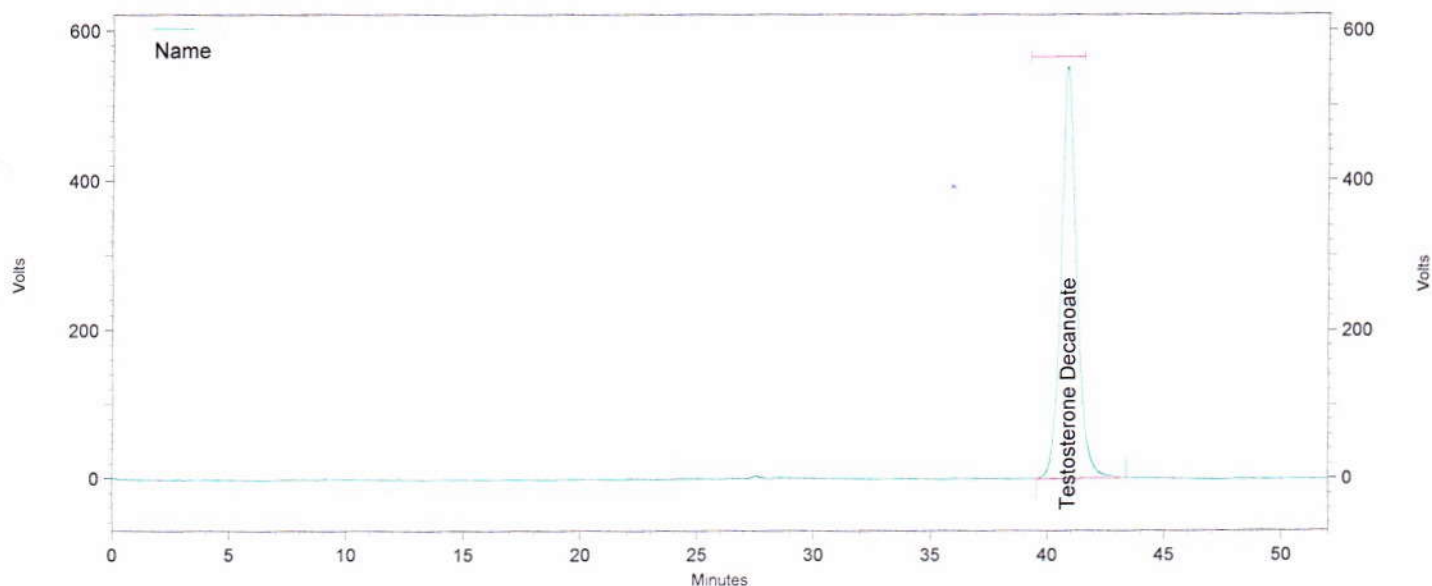

Channel A

UV Results


Name	Time	Area	Amount	Area Percent
Testosterone propionate			0,000 BDL	
Testosterone Phenylpropionate			0,000 BDL	
Testosterone isocaproate			0,000 BDL	
Testosterone Decanoate	40,847	102784795	0,000	100,000
Totals		102784795	0,000	100,000

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2015\August 2015\Diverse Steroide\18,08,15\24.08.2015 10-48-54_C34814 A-Rep2.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC: Nr.5
 Analysendatum: 24.08.2015 11:43:30
 Vial: 40
 Probenidentifikation: C34814 B
 Operator: admin
 Chrom.-Beding. ACN / Wasser, gradient
 Temperatur: 40 °C
 Säule Nr. 88, 250 x 4,6, C18
 Detektion: UV 240nm

Druckdatum: 24.08.2015 17:24:52
 Injektvolumen: 20

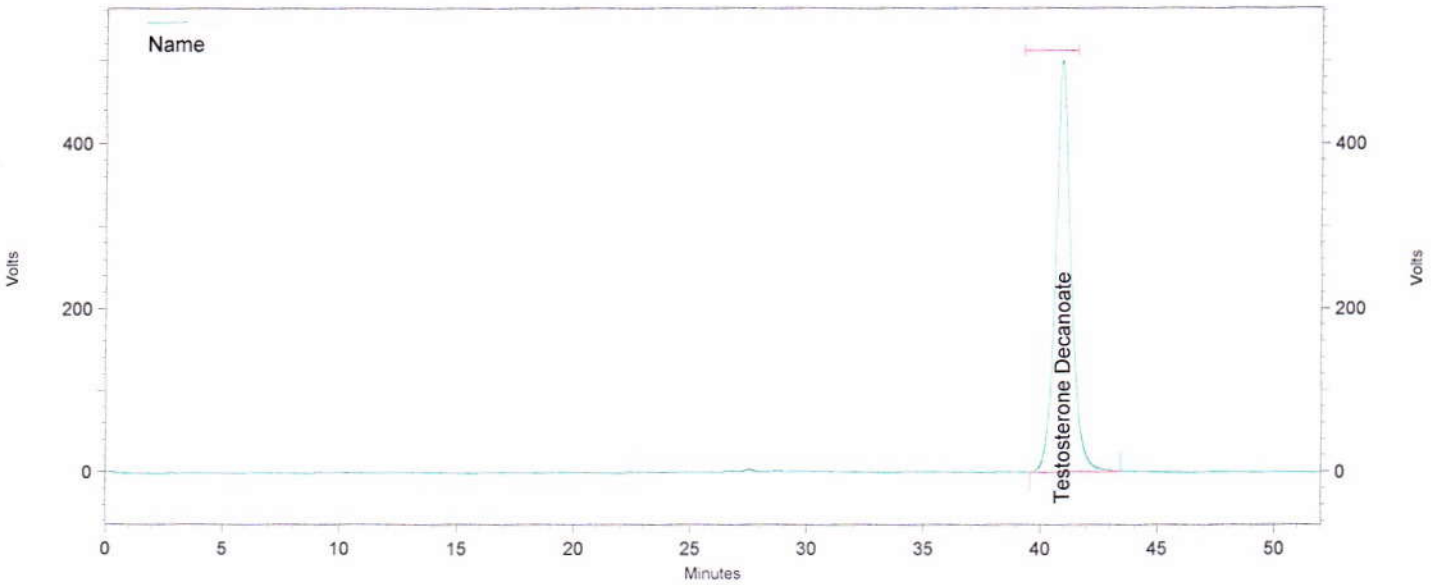

Channel A

UV Results


Name	Time	Area	Amount	Area Percent
Testosterone propionate			0,000 BDL	
Testosterone Phenylpropionate			0,000 BDL	
Testosterone isocaproate			0,000 BDL	
Testosterone Decanoate	40,910	92195944	0,000	100,000
Totals		92195944	0,000	100,000

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2015\August 2015\Diverse Steroide\18,08,15\24.08.2015 11-42-17_C34814 B-Rep1.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC: Nr.5
 Analysendatum: 24.08.2015 12:36:55
 Vial: 40
 Probenidentifikation: C34814 B
 Operator: admin
 Chrom.-Beding.: ACN / Wasser, gradient
 Temperatur: 40 °C
 Säule: Nr. 88, 250 x 4,6, C18
 Detektion: UV 240nm

Druckdatum: 24.08.2015 17:25:02
 Injektvolumen: 20

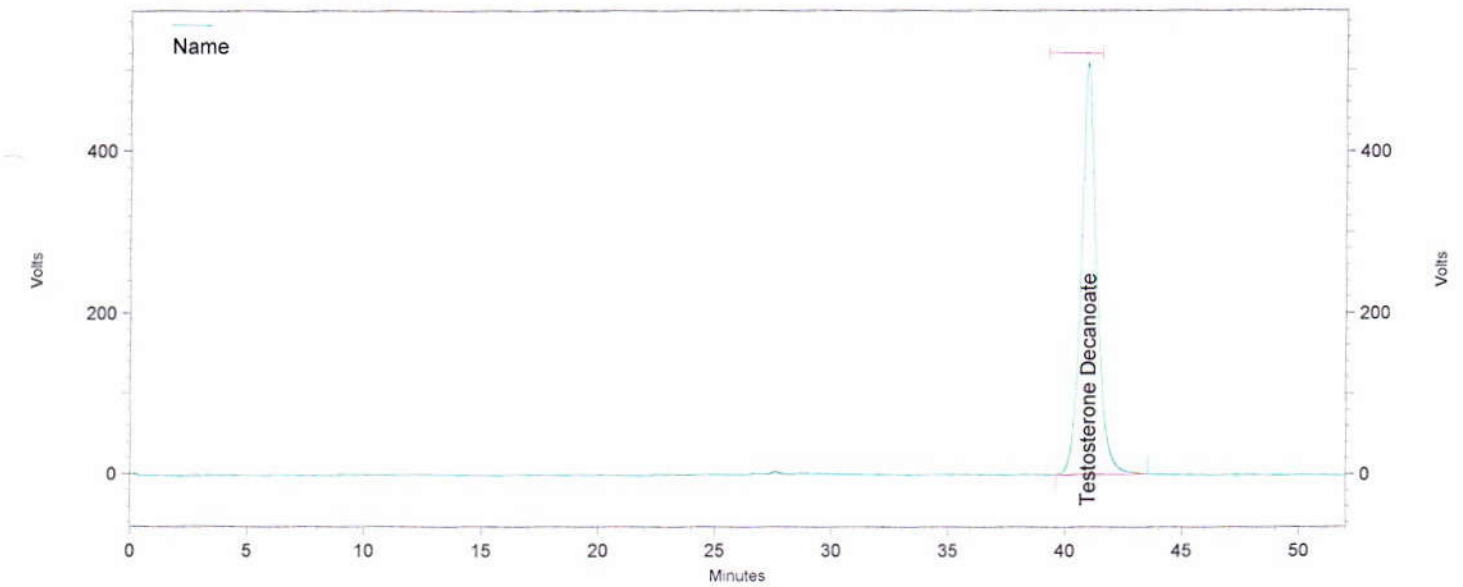

Channel A

UV Results


Name	Time	Area	Amount	Area Percent
Testosterone propionate			0,000 BDL	
Testosterone Phenylpropionate			0,000 BDL	
Testosterone isocaproate			0,000 BDL	
Testosterone Decanoate	40,950	94208882	0,000	100,000
Totals		94208882	0,000	100,000

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2015\August 2015\Diverse Steroide\18,08,15\24.08.2015 12-35-43_C34814 B-Rep2.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC: Nr.5
 Analysendatum: 24.08.2015 13:30:18
 Vial: 40
 Probenidentifikation: C34814 B
 Operator: admin
 Chrom.-Beding.: ACN / Wasser, gradient
 Temperatur: 40 °C
 Säule: Nr. 88, 250 x 4,6, C18
 Detektion: UV 240nm

Druckdatum: 24.08.2015 17:25:27
 Injektvolumen: 20

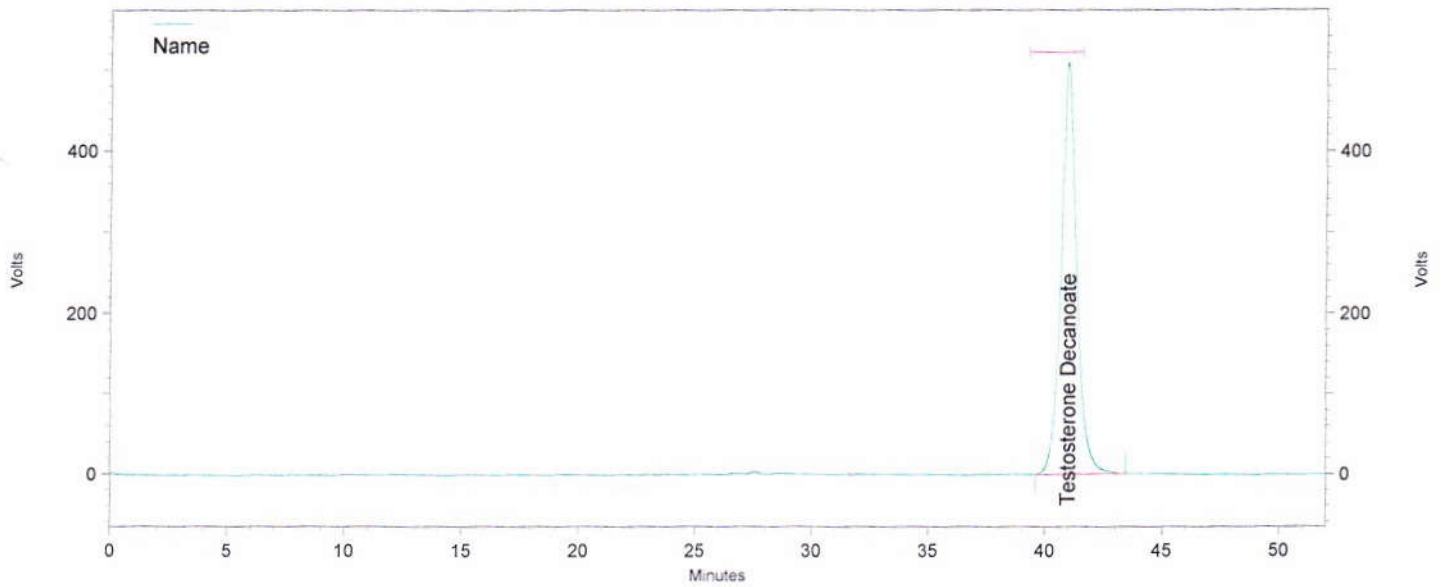

Channel A

UV Results

Name	Time	Area	Amount	Area Percent
Testosterone propionate			0,000 BDL	
Testosterone Phenylpropionate			0,000 BDL	
Testosterone isocaproate			0,000 BDL	
Testosterone Decanoate	40,950	94450501	0,000	100,000
Totals		94450501	0,000	100,000

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2015\August 2015\Diverse Steroide\18,08,15\24.08.2015 13-29-02_C34814 B-Rep3.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met